



Direct Nasopharyngeal Swab Procedure

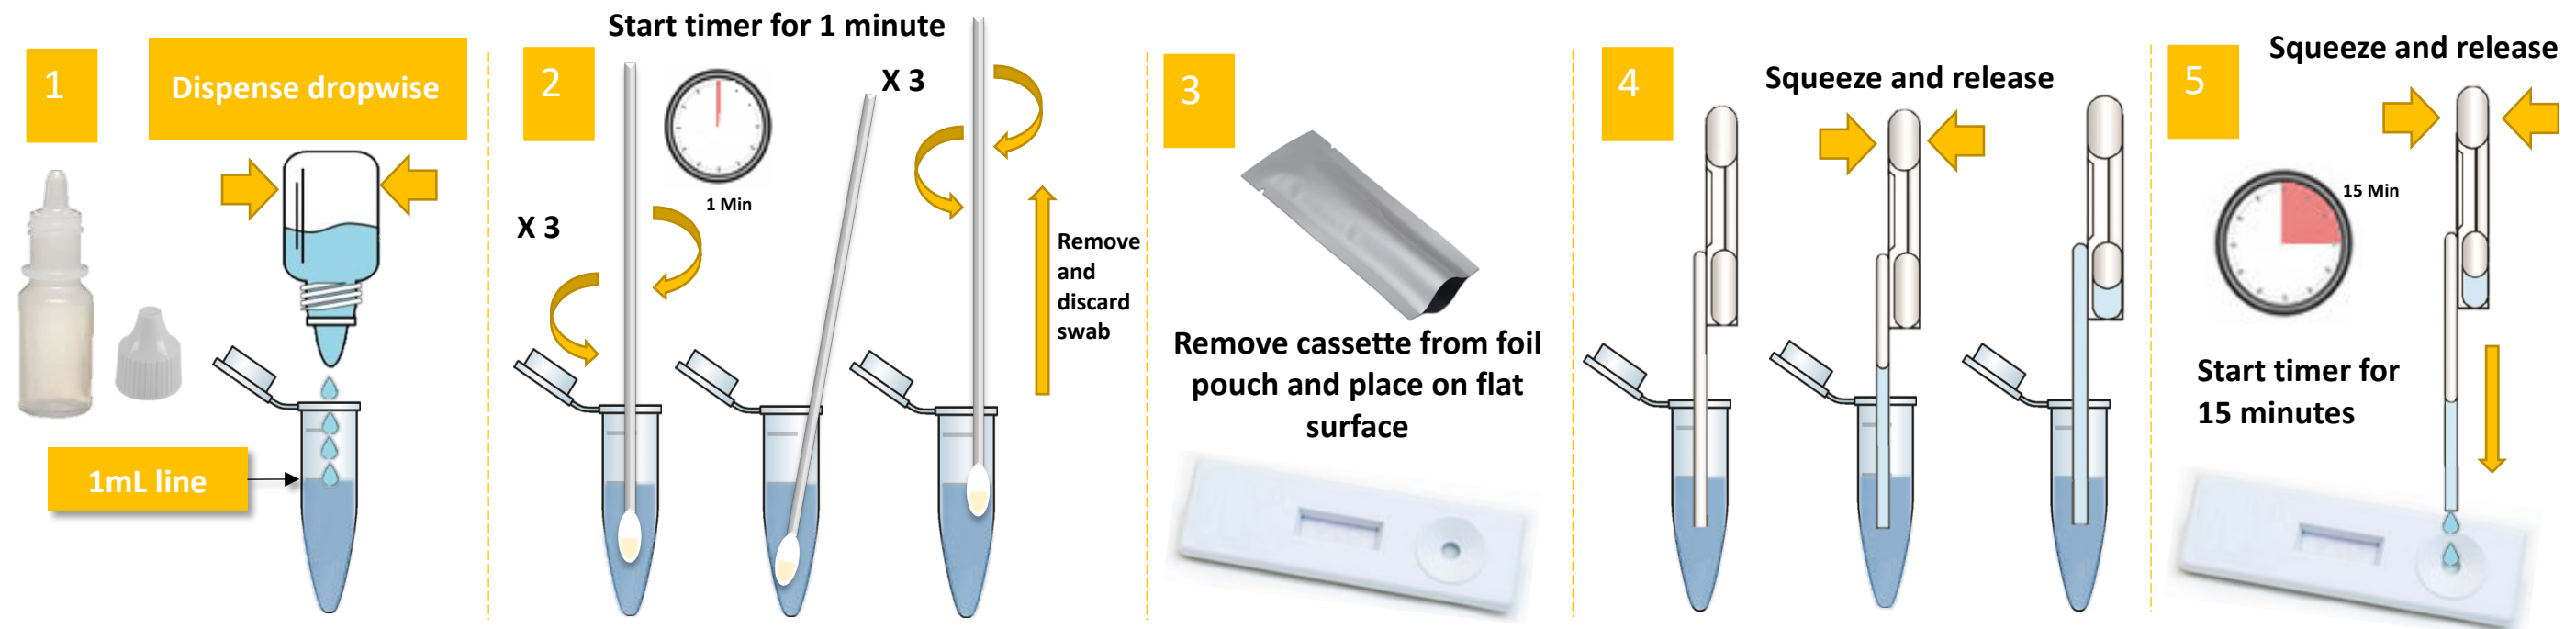


Positive

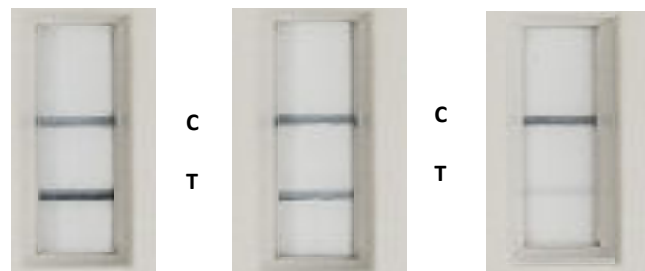

Negative



Invalid

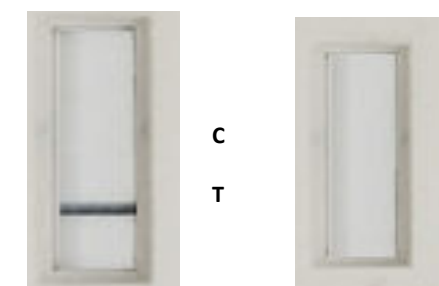

T = COVID-19 Test Line

C = Control Line



Consult Instructions for Use



OBELIS S.A
Bd. General Wahis, 53, 1030 Brussels, Belgium.
E-mail: mail@obelis.net
TEL: +32-2-732-59-54 FAX: +32-2-732-60-03



Sona Nanotech
Dartmouth, NS B2Y 4M9 Canada
Sonanano.com

External Control Dropper Bottle Procedure

1

Positive Control




Negative Control



2




15 Min

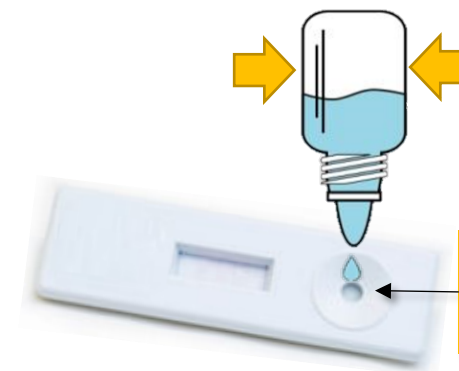

**Dispense
4 Drops**


Positive

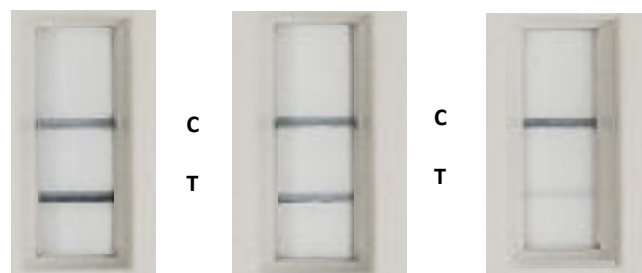

Negative



Invalid

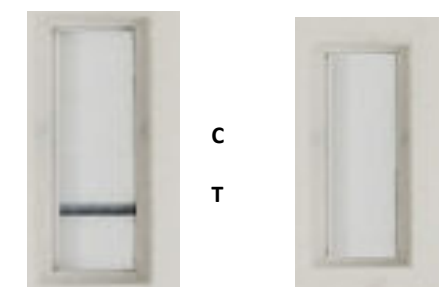

T = COVID-19 Test Line

C = Control Line



Consult Instructions for Use



OBELIS S.A
Bd. General Wahis, 53, 1030 Brussels, Belgium.
E-mail: mail@obelis.net
TEL: +32-2-732-59-54 FAX: +32-2-732-60-03



Sona Nanotech
Dartmouth, NS B2Y 4M9 Canada
Sonanano.com